

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Wechselland Alpaka/Fritz Wagner  
Tauchen am Wechsel 61  
Tauchen am Wechsel 7421 Austria

03/03/15

Test No: 497775


### Animal and Sample Description

**Animal Name:** AOG Wowfaktor  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn

**Animal ID:** 900200000027542  
**Sample Location:** Side (R)  
**Sample Date:** 02/08/15  
**Age:** 06/24/11

### Laboratory Data

**Mean Fiber Diameter:** 24.2 microns  
**Standard Deviation:** 5.1 microns  
**Coefficient of Variation:** 21.0 %  
**Fibers Greater Than 30 microns:** 9.0 %

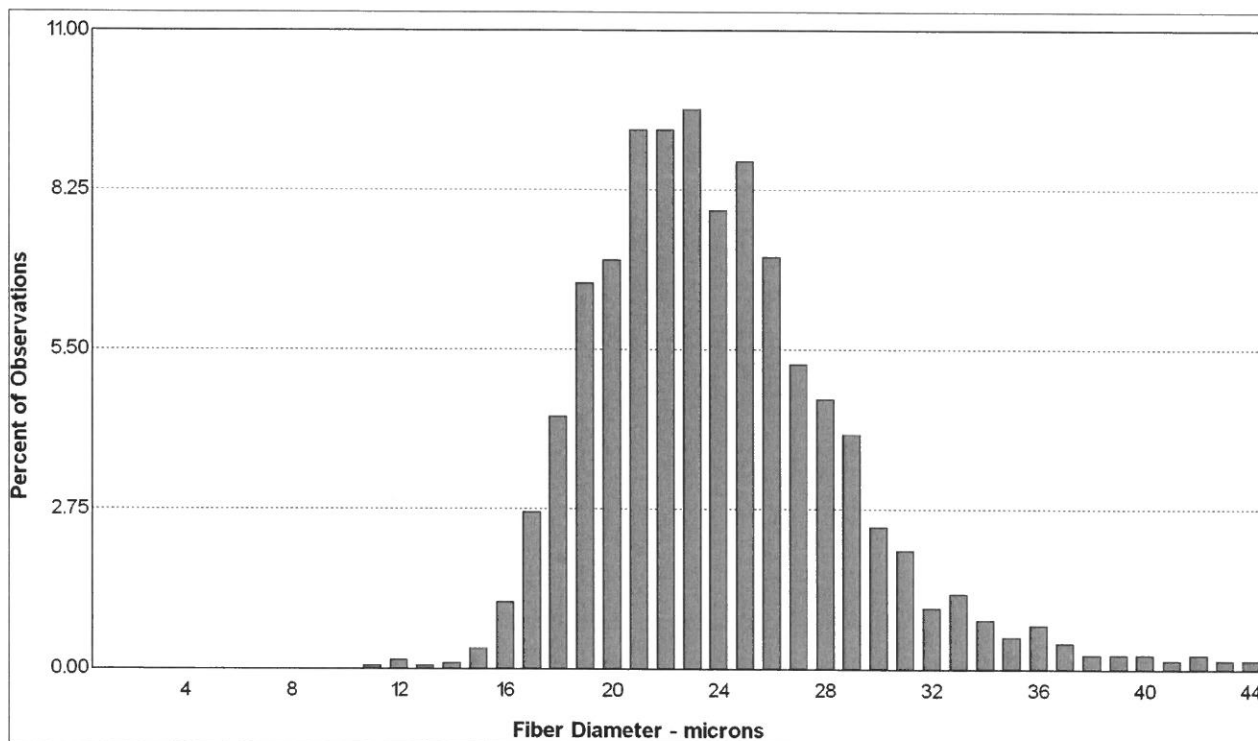

This Test Performed According to I.W.T.O Method 12