

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alpakas vom Silberberg/Pia Schindler
Freiberger Straße 40
Lengefeld 09514 Germany

04/18/13

Test No: 451930


Animal and Sample Description

Animal Name: ASB Alemandra
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/01/13
Age: 08/02/12

Laboratory Data

Mean Fiber Diameter:	18.2 microns	Spin Fineness:	17.5 microns
Standard Deviation:	3.5 microns	Mean Curvature (deg/mm):	33.3
Coefficient of Variation:	19.1 %	SD Curvature (deg/mm):	24.3
Fibers Greater Than 30 microns:	0.7 %	Comfort Factor:	99.3 %
Medullated Fibers:	6.1 %		

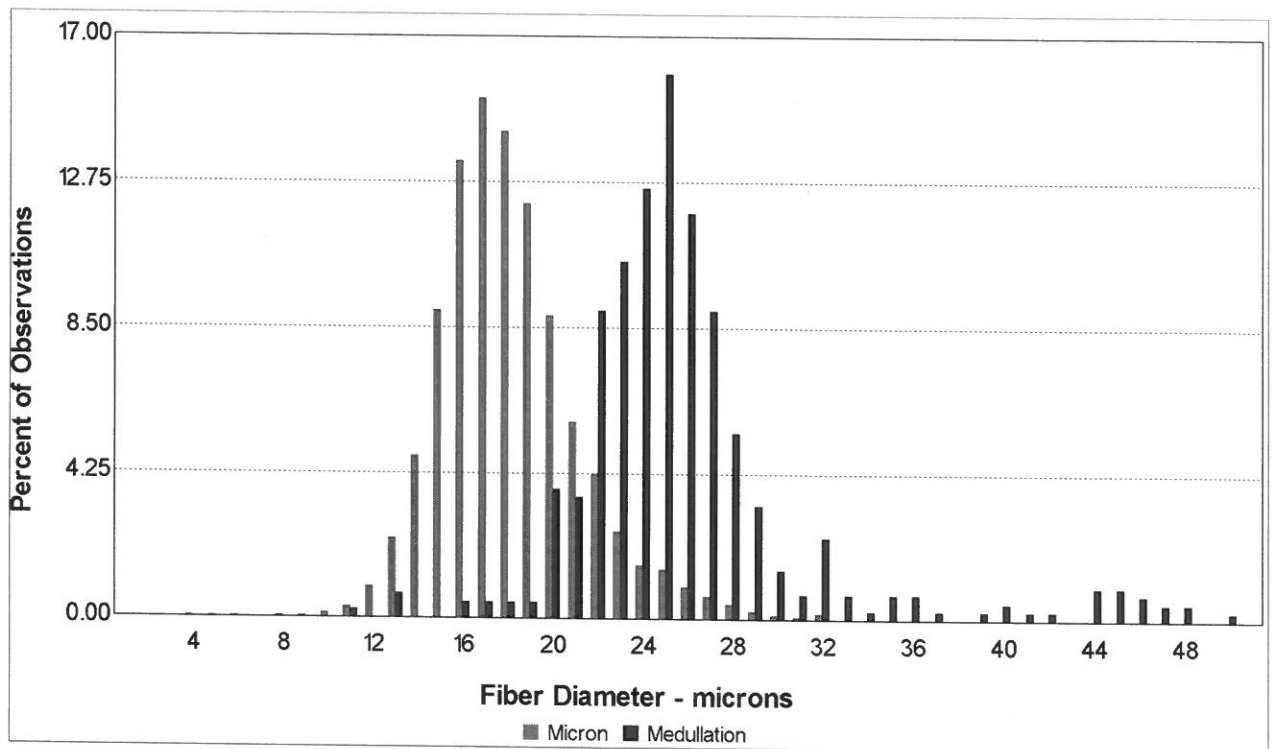

This Test Performed According to I.W.T.O Method 47