



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

08/08/17

Test No: 947070


Animal and Sample Description

Animal Name: ASB Arctic Maxima
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 276094180055146
Sample Location: Side (R)
Sample Date: 04/28/17
Age: 05/18/11

Laboratory Data

Mean Fiber Diameter:	20.3 microns	Spin Fineness:	19.3 microns
Standard Deviation:	3.8 microns	Mean Curvature (deg/mm):	54.9
Coefficient of Variation:	18.6 %	SD Curvature (deg/mm):	36.2
Fibers Greater Than 30 microns:	1.6 %	Comfort Factor:	98.4 %

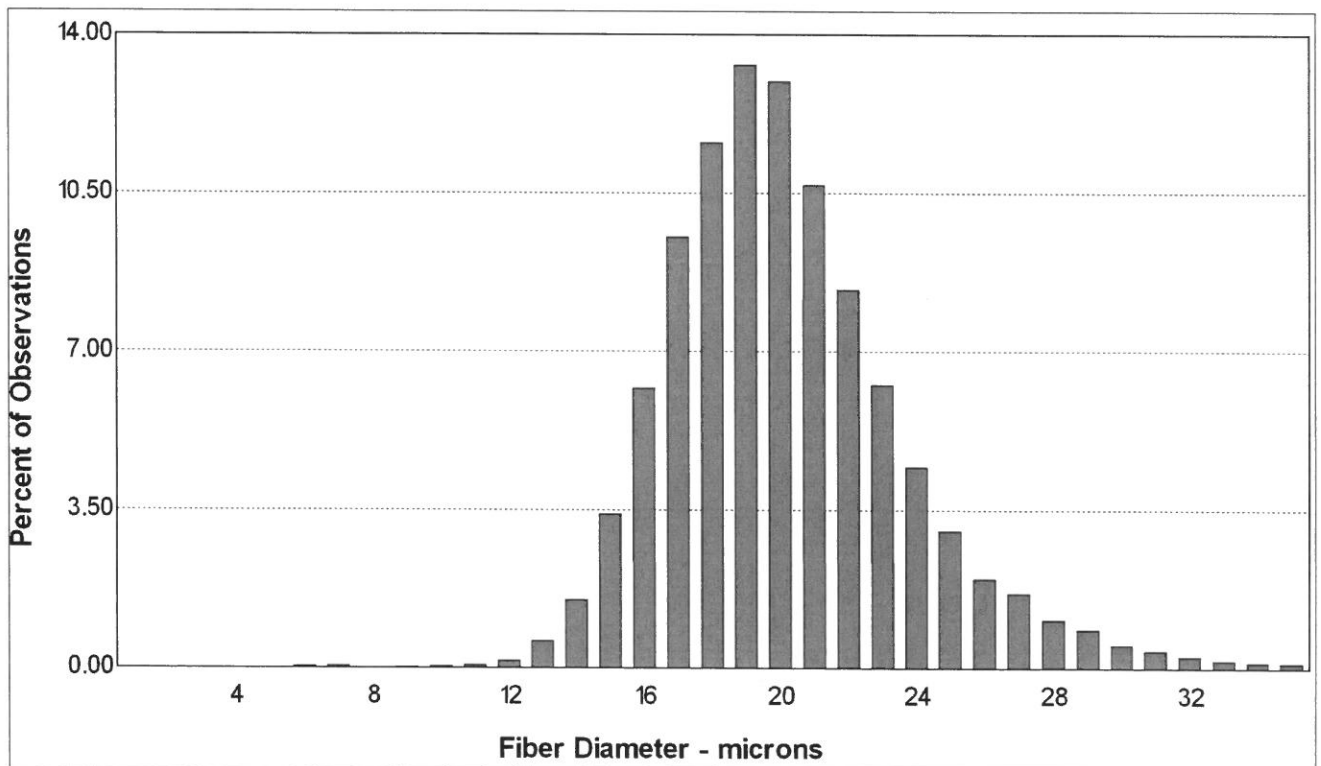

This Test Performed According to I.W.T.O Method 47