



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

06/13/18

Test No: 961512


Animal and Sample Description

Animal Name: JAW Venus
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 40100000032173
Sample Location: Side (R)
Sample Date: 04/22/18
Age: 10/02/13

Laboratory Data

Mean Fiber Diameter:	20.4 microns	Spin Fineness:	19.6 microns
Standard Deviation:	3.9 microns	Mean Curvature (deg/mm):	44.9
Coefficient of Variation:	18.9 %	SD Curvature (deg/mm):	26.5
Fibers Greater Than 30 microns:	1.5 %	Comfort Factor:	98.5 %

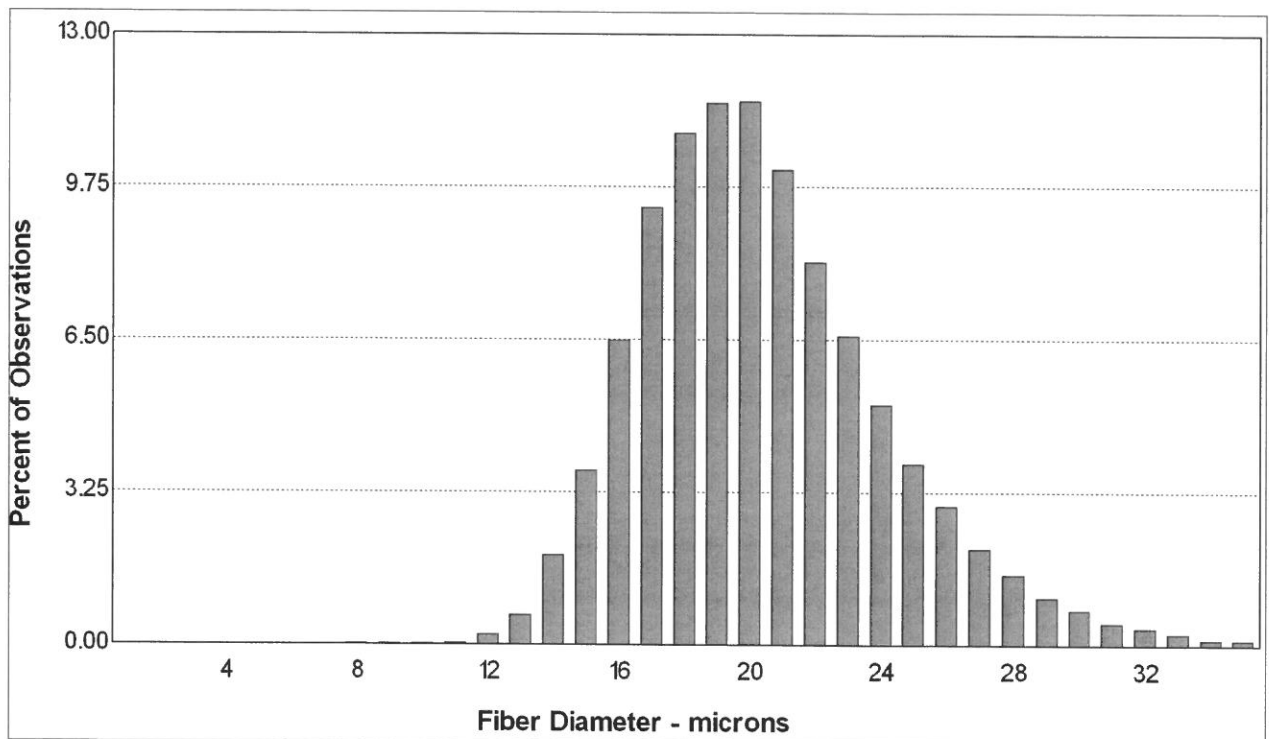

This Test Performed According to I.W.T.O Method 47