



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer
Tauchen am Wechsel 61
7421 Tauchen am Wechsel Austria

Date: 02/18/19

Test No: 972714


Animal and Sample Description

Animal Name: JAW Venus
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 4010000032173
Sample Location: Side
Sample Date: 02/03/19
Age: 10/03/13

Laboratory Data

| | | | |
|----------------------------------|--------------|--|-------------|
| Mean Fiber Diameter: | 22.8 microns | Fibers Greater Than 30 microns: | 4.6 % |
| Standard Deviation: | 4.3 microns | Comfort Factor: | 95.4 % |
| Coefficient of Variation: | 19.0 % | Mean Curvature: | 38.4 deg/mm |
| Spin Fineness: | 21.8 microns | SD Curvature: | 22.8 deg/mm |

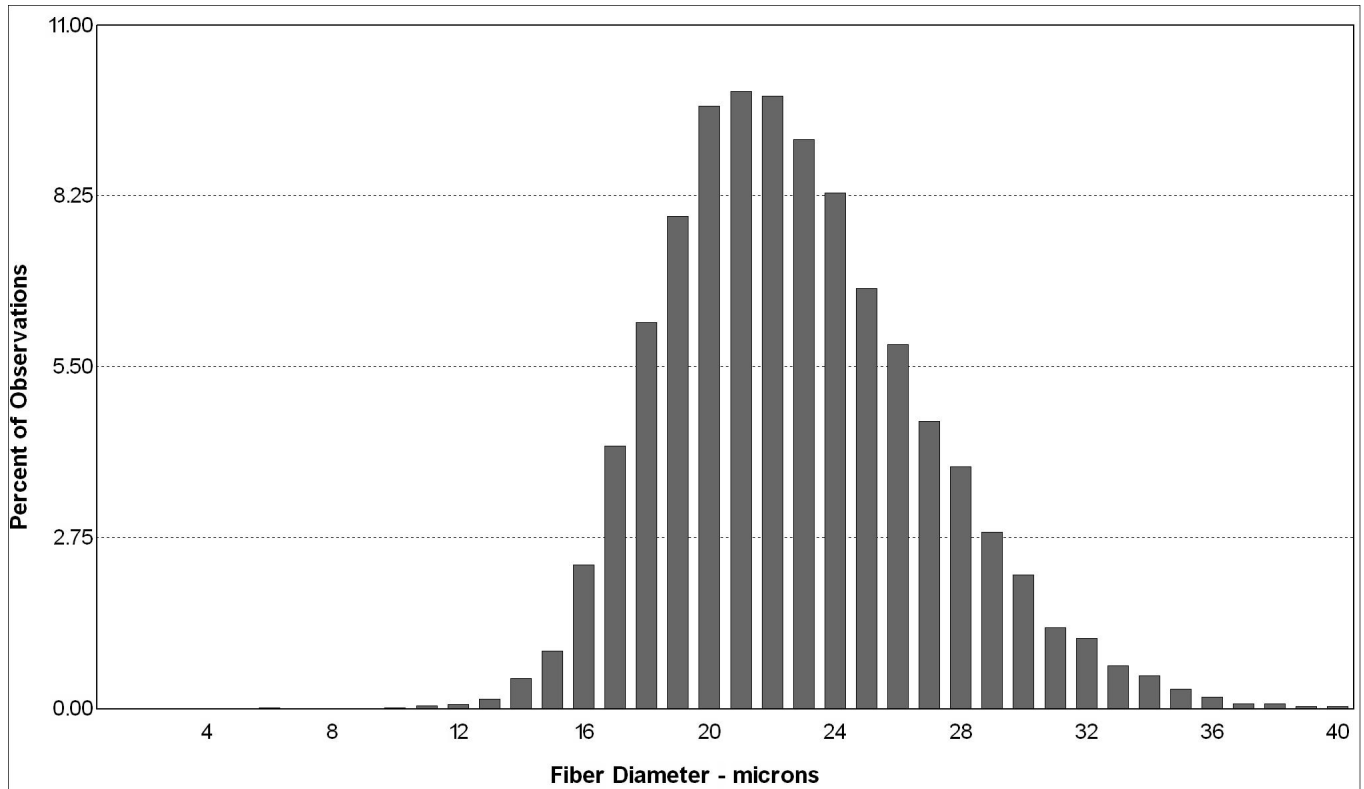

This Test Performed According to I.W.T.O Method 47