



## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Wechselland Alpaka/Fritz Wagner  
Tauchen am Wechsel 61  
Tauchen am Wechsel 7421 Austria

03/03/15

Test No: 497770


#### Animal and Sample Description

**Animal Name:** MMR Venola  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Animal ID:** 941000001913479  
**Sample Location:** Side (R)  
**Sample Date:** 02/08/15  
**Age:** 06/17/07

#### Laboratory Data

**Mean Fiber Diameter:** 22.1 microns  
**Standard Deviation:** 4.7 microns  
**Coefficient of Variation:** 21.1 %  
**Fibers Greater Than 30 microns:** 6.4 %

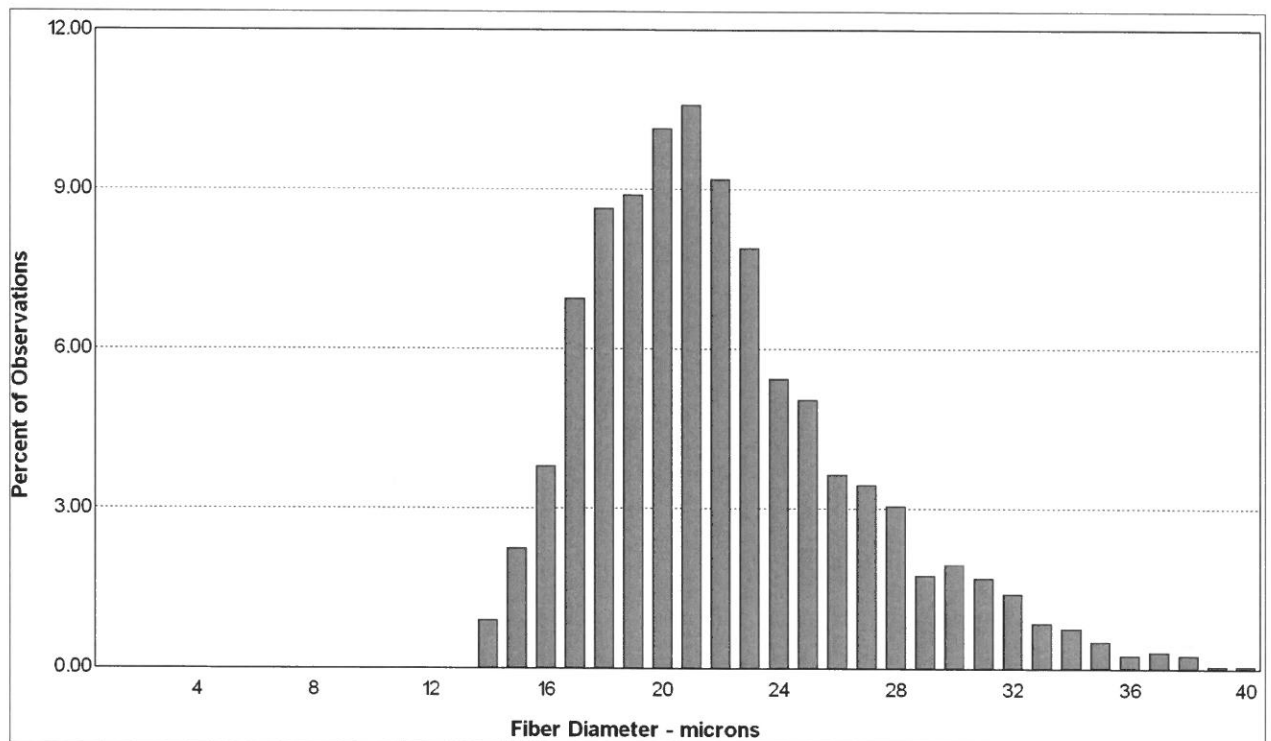

This Test Performed According to I.W.T.O Method 12