



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

08/08/17

Test No: 947078


Animal and Sample Description

Animal Name: SNOWMASS Elite Legacy XX
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: 756098100702147
Sample Location: Side (R)
Sample Date: 04/28/17
Age: 08/29/07

Laboratory Data

Mean Fiber Diameter:	21.3 microns	Spin Fineness:	21.1 microns
Standard Deviation:	4.9 microns	Mean Curvature (deg/mm):	41.8
Coefficient of Variation:	22.7 %	SD Curvature (deg/mm):	27.2
Fibers Greater Than 30 microns:	5.0 %	Comfort Factor:	95.0 %

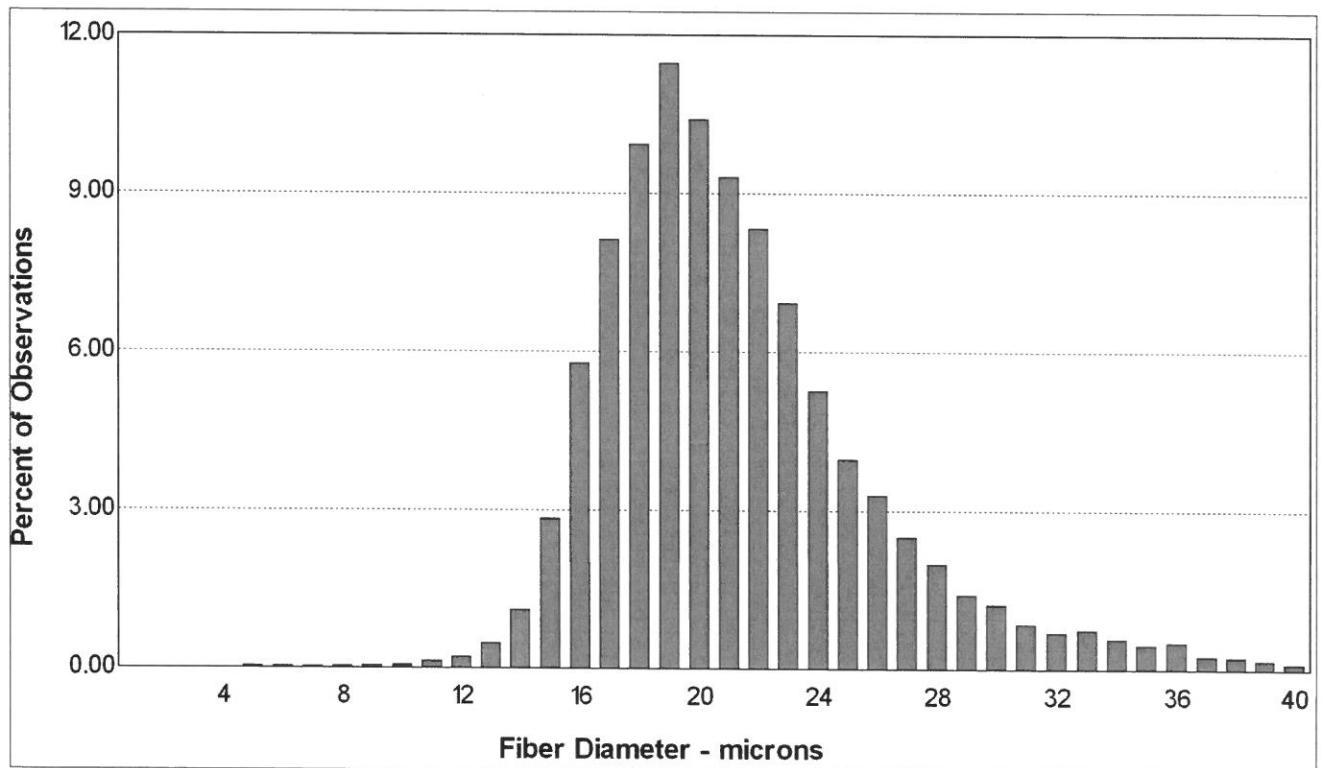

This Test Performed According to I.W.T.O Method 47