



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner  
Tauchen 61  
7421 Tauchen am Wechsel NÖ Austria

06/13/18

Test No: 961498


### Animal and Sample Description

**Animal Name:** Snowmass Elite Legacy XX  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Beige

**Animal ID:** 756098100702147  
**Sample Location:** Side (R)  
**Sample Date:** 04/22/18  
**Age:** 08/29/07

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.8 microns	<b>Spin Fineness:</b>	22.6 microns
<b>Standard Deviation:</b>	4.3 microns	<b>Mean Curvature (deg/mm):</b>	40.0
<b>Coefficient of Variation:</b>	18.2 %	<b>SD Curvature (deg/mm):</b>	22.2
<b>Fibers Greater Than 30 microns:</b>	6.6 %	<b>Comfort Factor:</b>	93.4 %

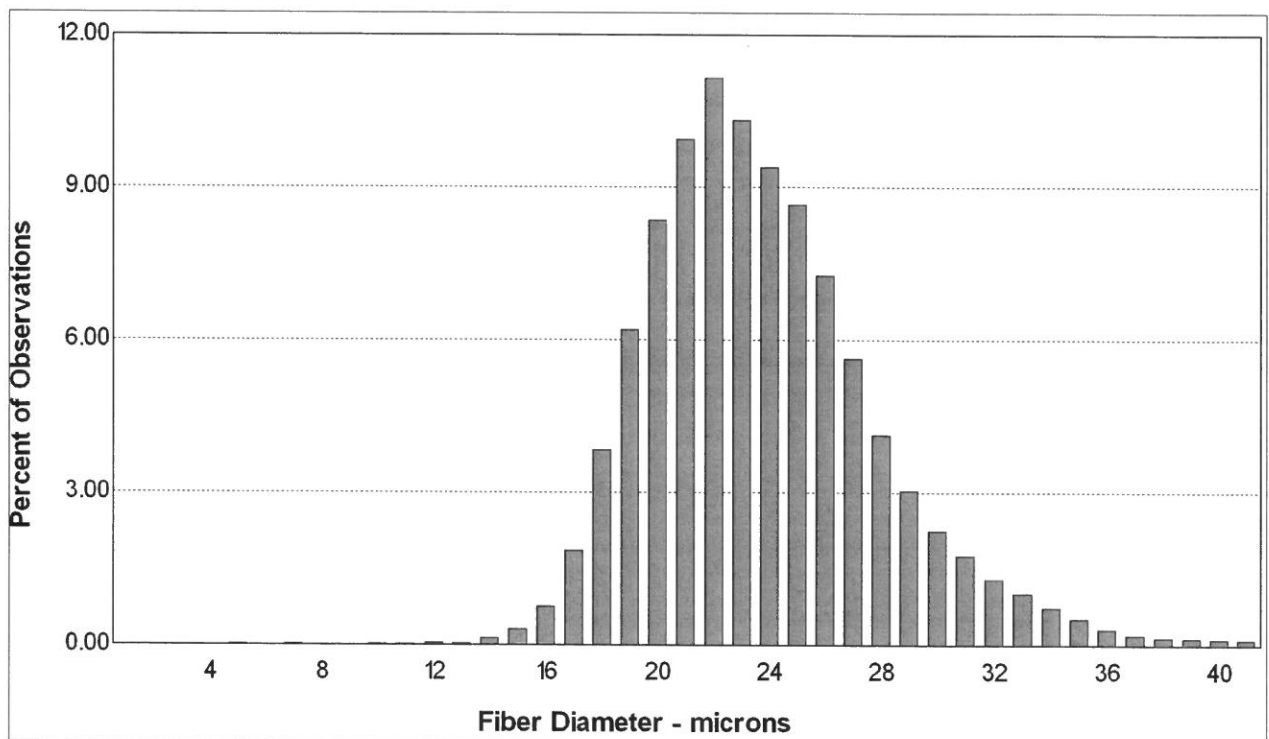

This Test Performed According to I.W.T.O Method 47