



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer
Tauchen am Wechsel 61
7421 Tauchen am Wechsel Austria

Date: 02/18/19

Test No: 972699


Animal and Sample Description

Animal Name: USA16 Snowmass Elite Legacy XX
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige CH756098100702147

Animal ID: 756098100702147
Sample Location: Side
Sample Date: 02/03/19
Age: 06/29/07

Laboratory Data

Mean Fiber Diameter:	25.0 microns	Fibers Greater Than 30 microns:	12.3 %
Standard Deviation:	5.1 microns	Comfort Factor:	87.7 %
Coefficient of Variation:	20.2 %	Mean Curvature:	34.2 deg/mm
Spin Fineness:	24.1 microns	SD Curvature:	19.7 deg/mm

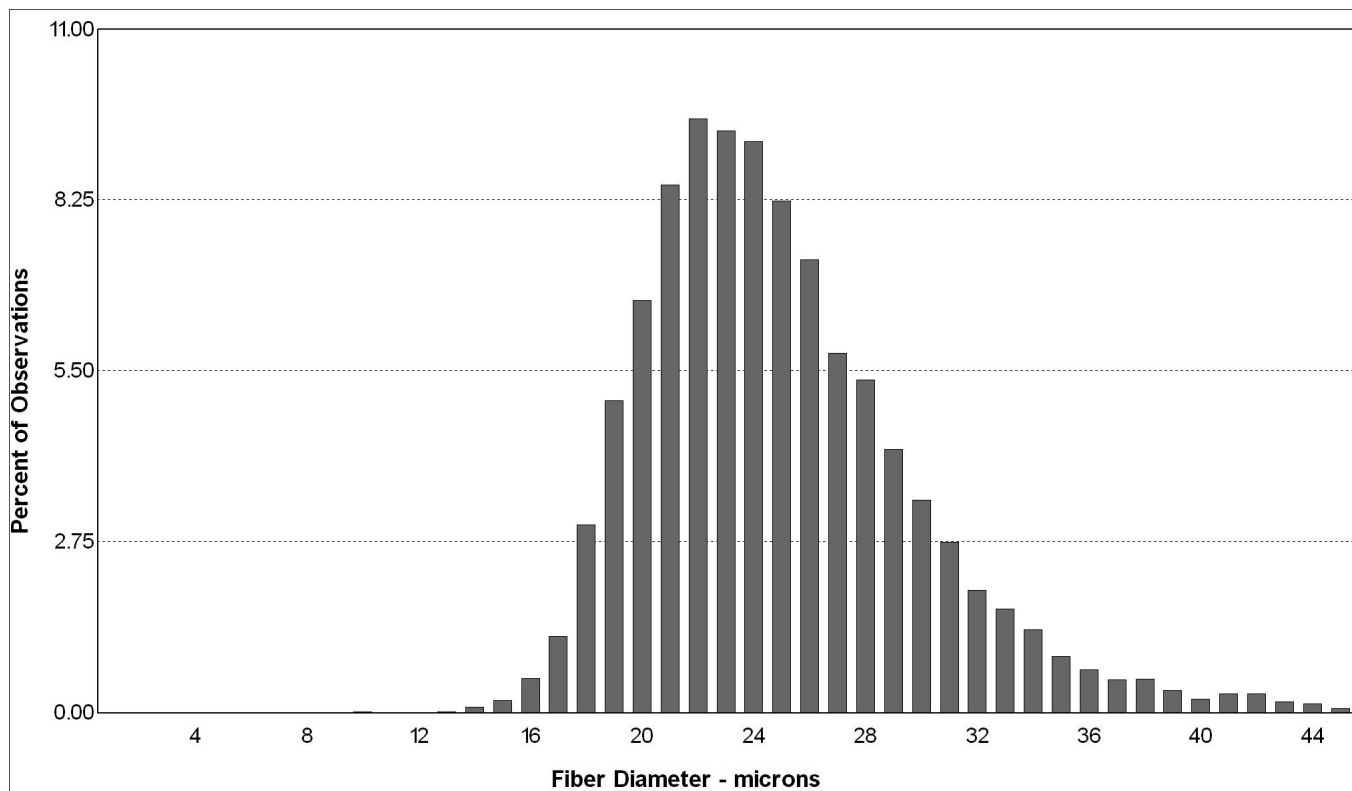

This Test Performed According to I.W.T.O Method 47