



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

WLA Wechselland Alpka/Fritz Wagner
Tauchen 61
Mönichkirchen 7421 Austria

03/13/20

Test No: 987879


Animal and Sample Description

Animal Name: Snowmass Elite Legacy XX
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: CH756098100702147
Sample Location: Side
Sample Date: 03/01/20
Age: 08/29/07

Laboratory Data

Mean Fiber Diameter:	22.5 microns	Spin Fineness:	21.7 microns
Standard Deviation:	4.5 microns	Medullated Fibers:	0.0 %
Coefficient of Variation:	20.2 %	Mean Curvature (deg/mm):	32.0
Fibers Greater Than 30 microns:	5.5 %	SD Curvature (deg/mm):	22.1

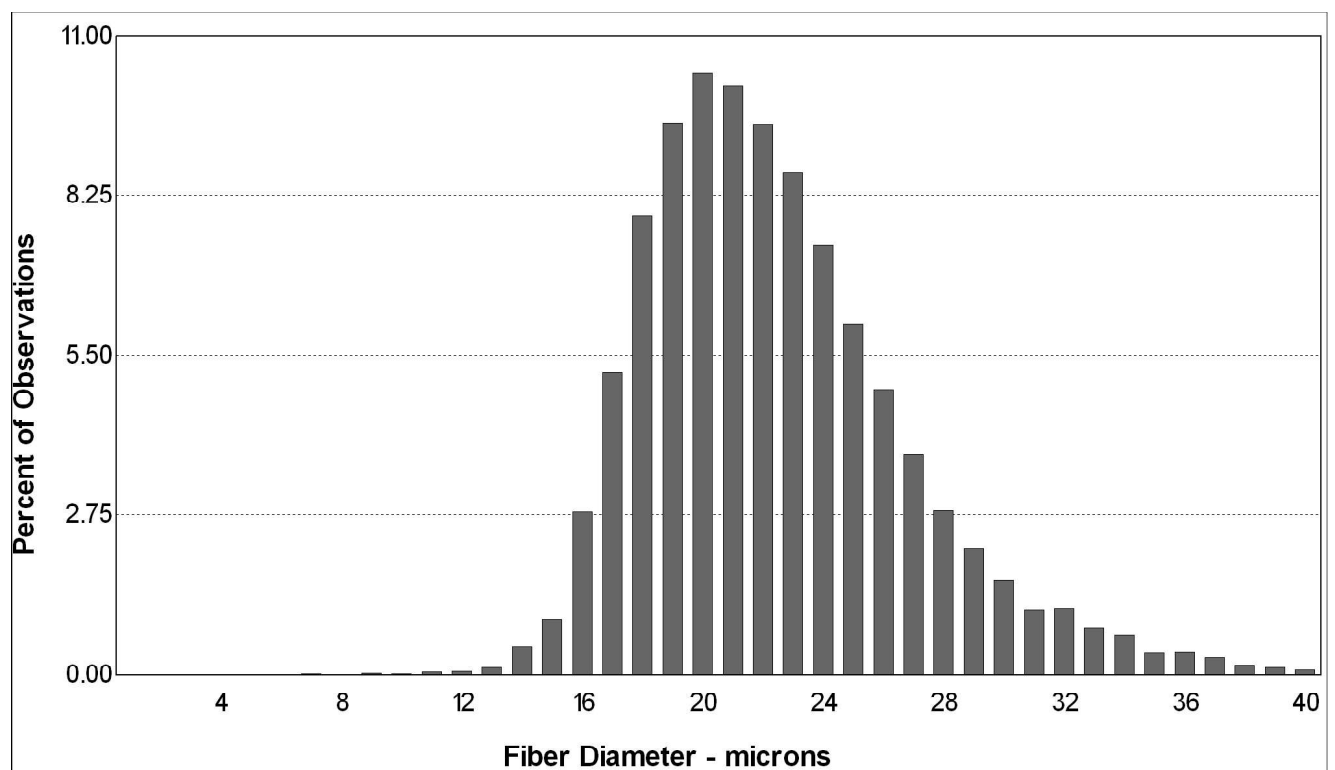

This Test Performed According to I.W.T.O Method 47