



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

WLA Wechselland Alpka/Fritz Wagner
Tauchen 61
Mönichkirchen 7421 Austria

03/13/20

Test No: 987872


Animal and Sample Description

Animal Name: WLA Abigale
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 276093400739355
Sample Location: Side
Sample Date: 03/01/20
Age: 06/13/19

Laboratory Data

Mean Fiber Diameter:	18.5 microns	Spin Fineness:	18.0 microns
Standard Deviation:	3.9 microns	Medullated Fibers:	0.0 %
Coefficient of Variation:	21.2 %	Mean Curvature (deg/mm):	42.3
Fibers Greater Than 30 microns:	1.2 %	SD Curvature (deg/mm):	26.2

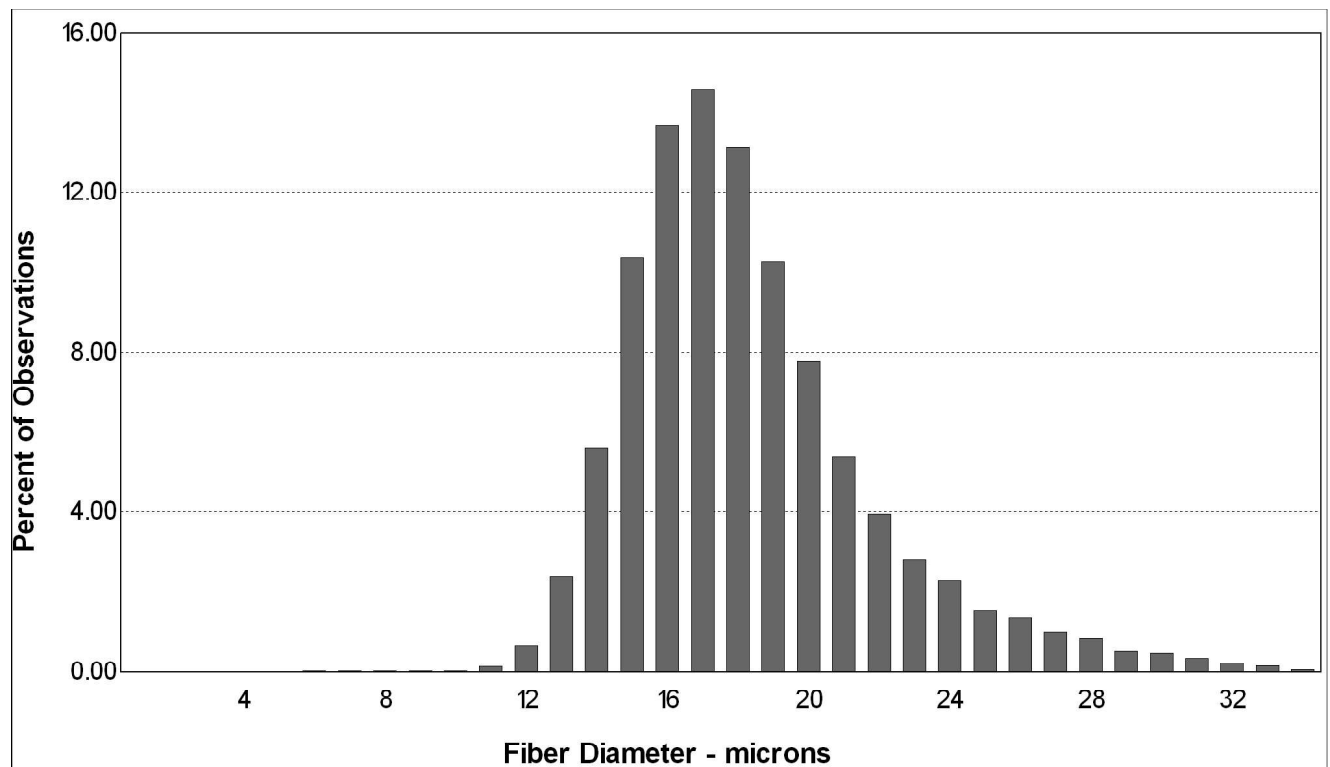

This Test Performed According to I.W.T.O Method 47