



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer
Tauchen am Wechsel 61
7421 Tauchen am Wechsel Austria

Date: 02/18/19

Test No: 972711


Animal and Sample Description

Animal Name: WLA May Flower
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 276093480007425
Sample Location: Side
Sample Date: 02/03/19
Age: 05/19/17

Laboratory Data

Mean Fiber Diameter:	23.8 microns	Fibers Greater Than 30 microns:	7.4 %
Standard Deviation:	4.8 microns	Comfort Factor:	92.6 %
Coefficient of Variation:	20.1 %	Mean Curvature:	33.1 deg/mm
Spin Fineness:	23.0 microns	SD Curvature:	19.1 deg/mm

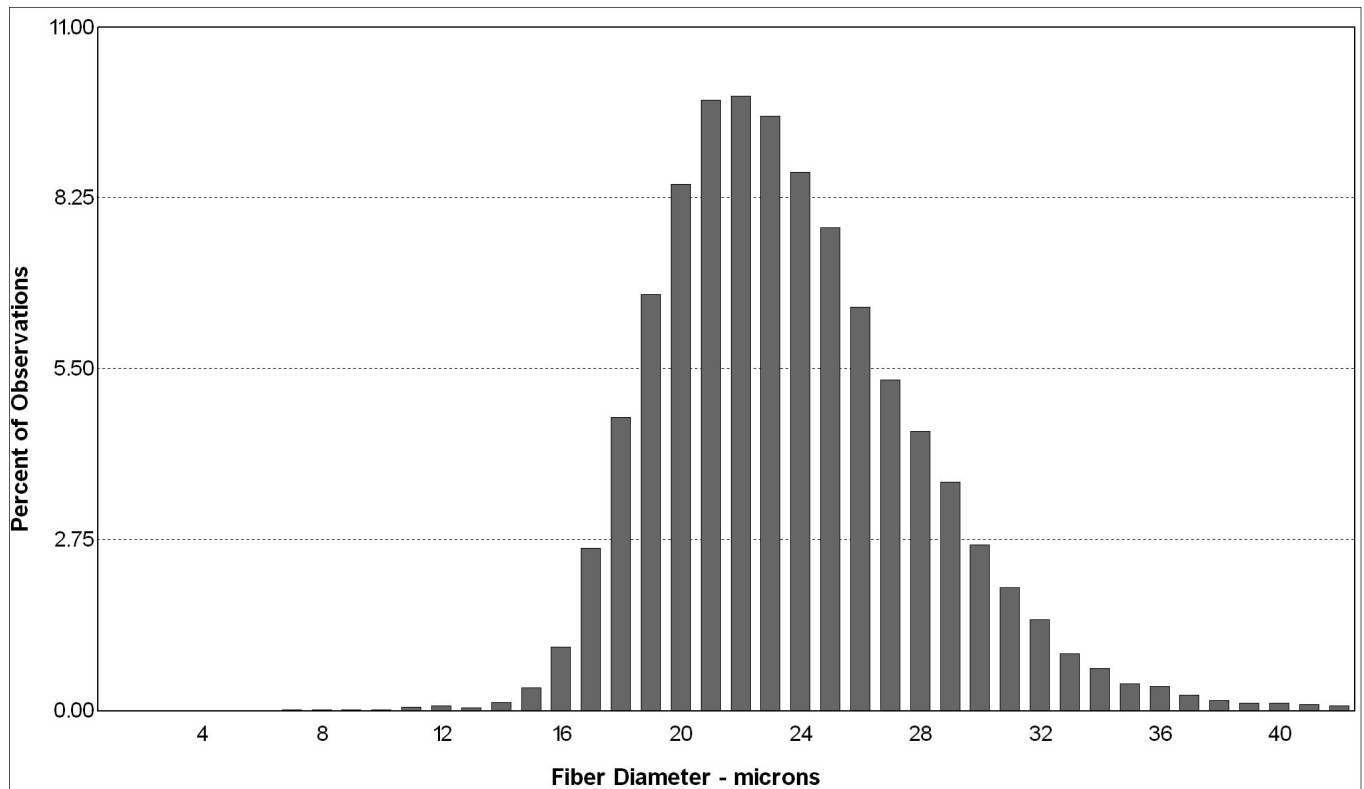

This Test Performed According to I.W.T.O Method 47