



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner  
Tauchen 61  
7421 Tauchen am Wechsel NÖ Austria

08/08/17

Test No: 947074


### Animal and Sample Description

**Animal Name:** WLA Precious Royal Pan  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** True Black

**Animal ID:** 276093480007427  
**Sample Location:** Side (R)  
**Sample Date:** 04/28/17  
**Age:** 05/26/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	16.7 microns	<b>Spin Fineness:</b>	16.5 microns
<b>Standard Deviation:</b>	3.9 microns	<b>Mean Curvature (deg/mm):</b>	40.7
<b>Coefficient of Variation:</b>	23.2 %	<b>SD Curvature (deg/mm):</b>	30.8
<b>Fibers Greater Than 30 microns:</b>	0.8 %	<b>Comfort Factor:</b>	99.2 %

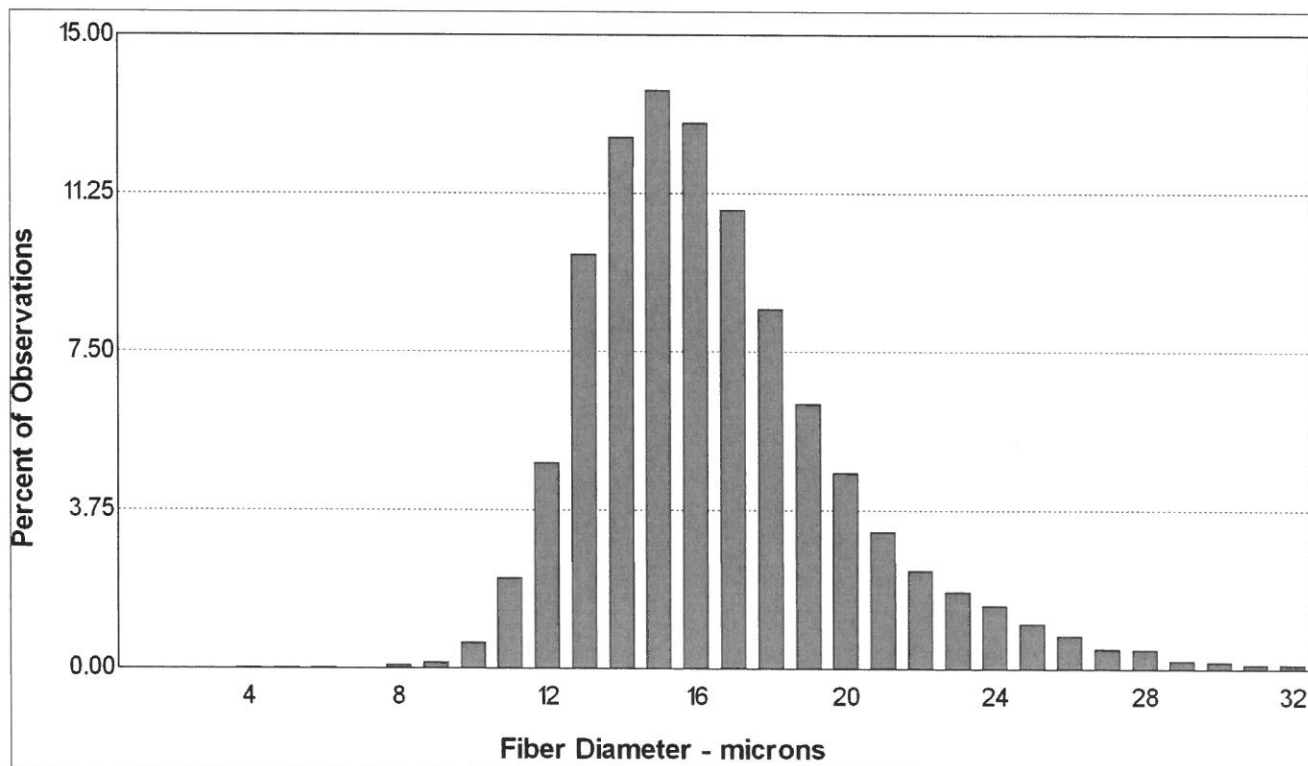

This Test Performed According to I.W.T.O Method 47