



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

06/13/18

Test No: 961499


Animal and Sample Description

Animal Name: WLA Raven
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 276093480007421
Sample Location: Side (R)
Sample Date: 04/22/18
Age: 05/14/17

Laboratory Data

Mean Fiber Diameter:	17.8 microns	Spin Fineness:	16.6 microns
Standard Deviation:	2.9 microns	Mean Curvature (deg/mm):	45.1
Coefficient of Variation:	16.2 %	SD Curvature (deg/mm):	33.0
Fibers Greater Than 30 microns:	0.2 %	Comfort Factor:	99.8 %

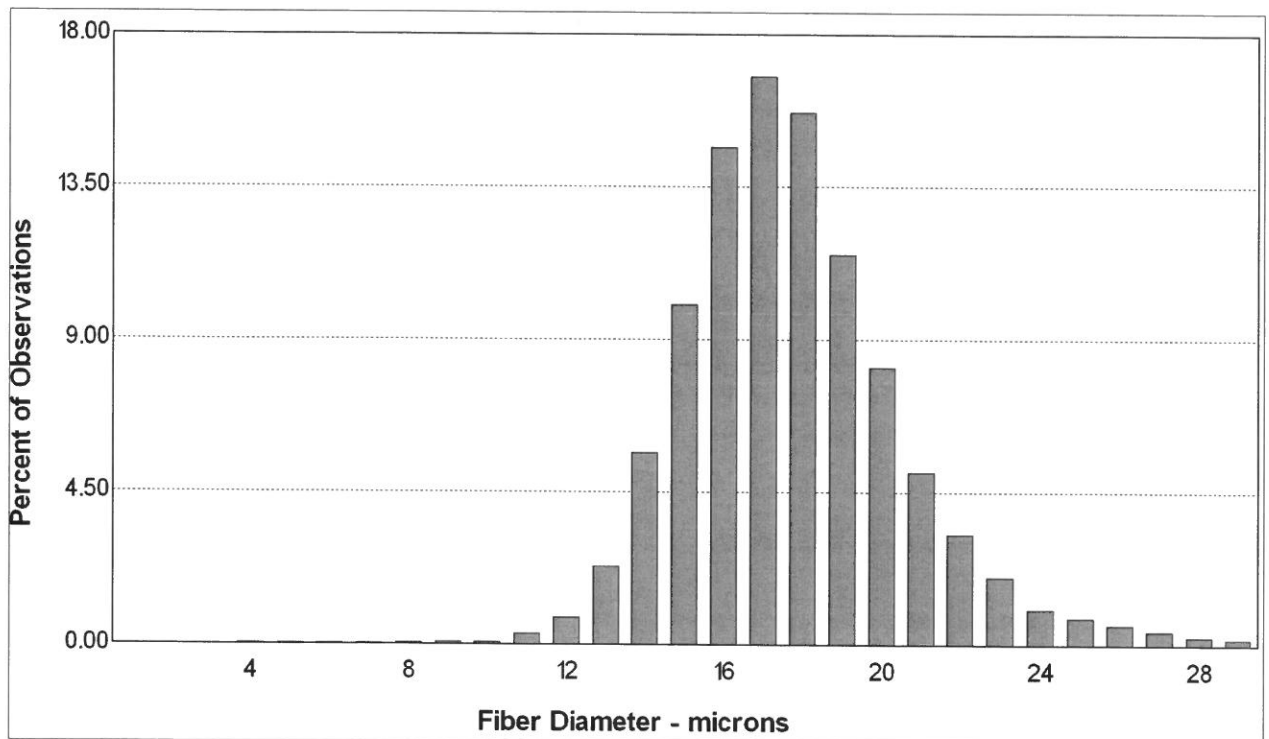

This Test Performed According to I.W.T.O Method 47