



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

WLA Wechselland Alpka/Fritz Wagner
Tauchen 61
Mönichkirchen 7421 Austria

03/13/20

Test No: 987882


Animal and Sample Description

Animal Name: WLA Vintage
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 276093400739485
Sample Location: Side
Sample Date: 03/01/20
Age: 07/09/19

Laboratory Data

Mean Fiber Diameter:	15.4 microns	Spin Fineness:	15.1 microns
Standard Deviation:	3.4 microns	Medullated Fibers:	0.0 %
Coefficient of Variation:	22.4 %	Mean Curvature (deg/mm):	57.5
Fibers Greater Than 30 microns:	0.4 %	SD Curvature (deg/mm):	31.0

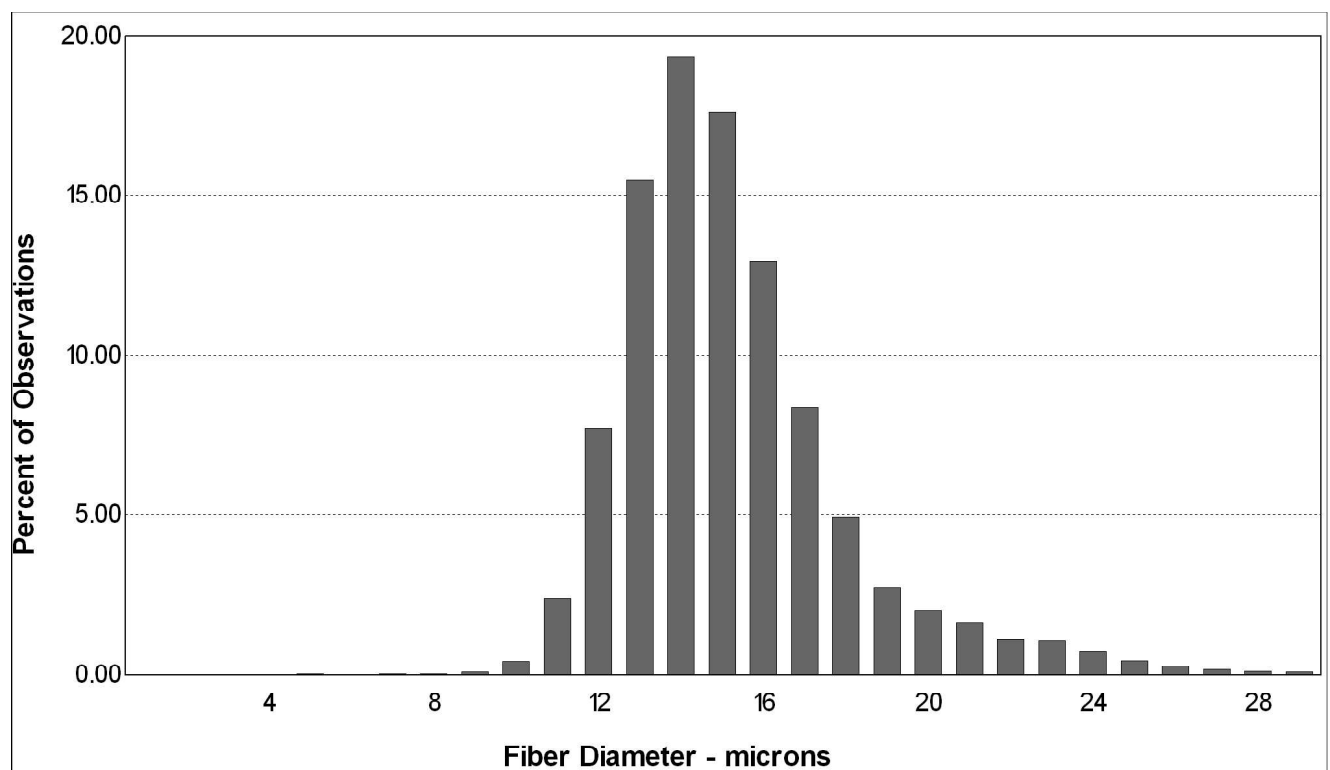

This Test Performed According to I.W.T.O Method 47