



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

08/08/17

Test No: 947081


Animal and Sample Description

Animal Name: DE15 Queen
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Silver Grey

Animal ID: 90020000080977
Sample Location: Side (R)
Sample Date: 04/28/17
Age: 07/12/13

Laboratory Data

Mean Fiber Diameter:	18.8 microns	Spin Fineness:	21.0 microns
Standard Deviation:	6.5 microns	Mean Curvature (deg/mm):	49.7
Coefficient of Variation:	34.6 %	SD Curvature (deg/mm):	39.4
Fibers Greater Than 30 microns:	7.5 %	Comfort Factor:	92.5 %

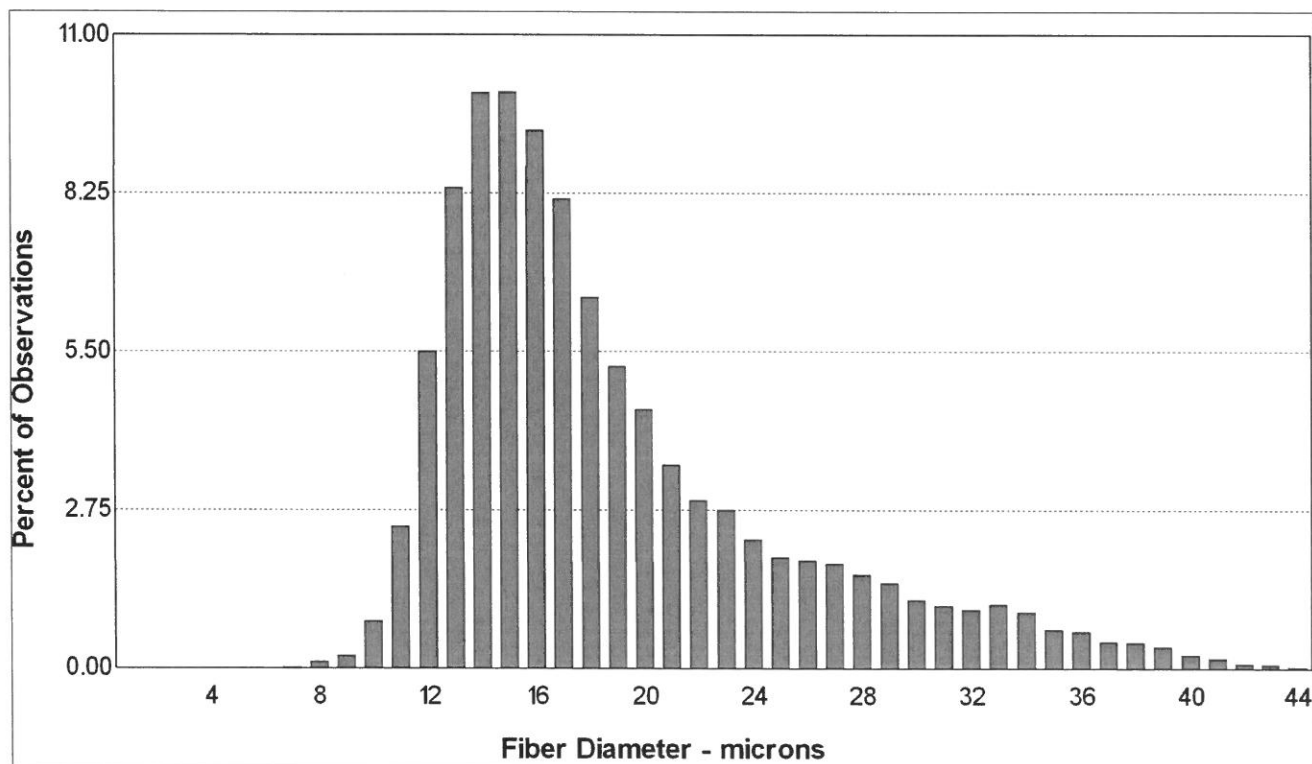

This Test Performed According to I.W.T.O Method 47