



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer
Tauchen am Wechsel 61
7421 Tauchen am Wechsel Austria

Date: 02/18/19

Test No: 972712


Animal and Sample Description

Animal Name: ZL Victoria
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 900200000098015
Sample Location: Side
Sample Date: 02/03/19
Age: 06/05/12

Laboratory Data

Mean Fiber Diameter:	21.3 microns	Fibers Greater Than 30 microns:	3.7 %
Standard Deviation:	4.3 microns	Comfort Factor:	96.3 %
Coefficient of Variation:	20.3 %	Mean Curvature:	45.0 deg/mm
Spin Fineness:	20.6 microns	SD Curvature:	26.4 deg/mm

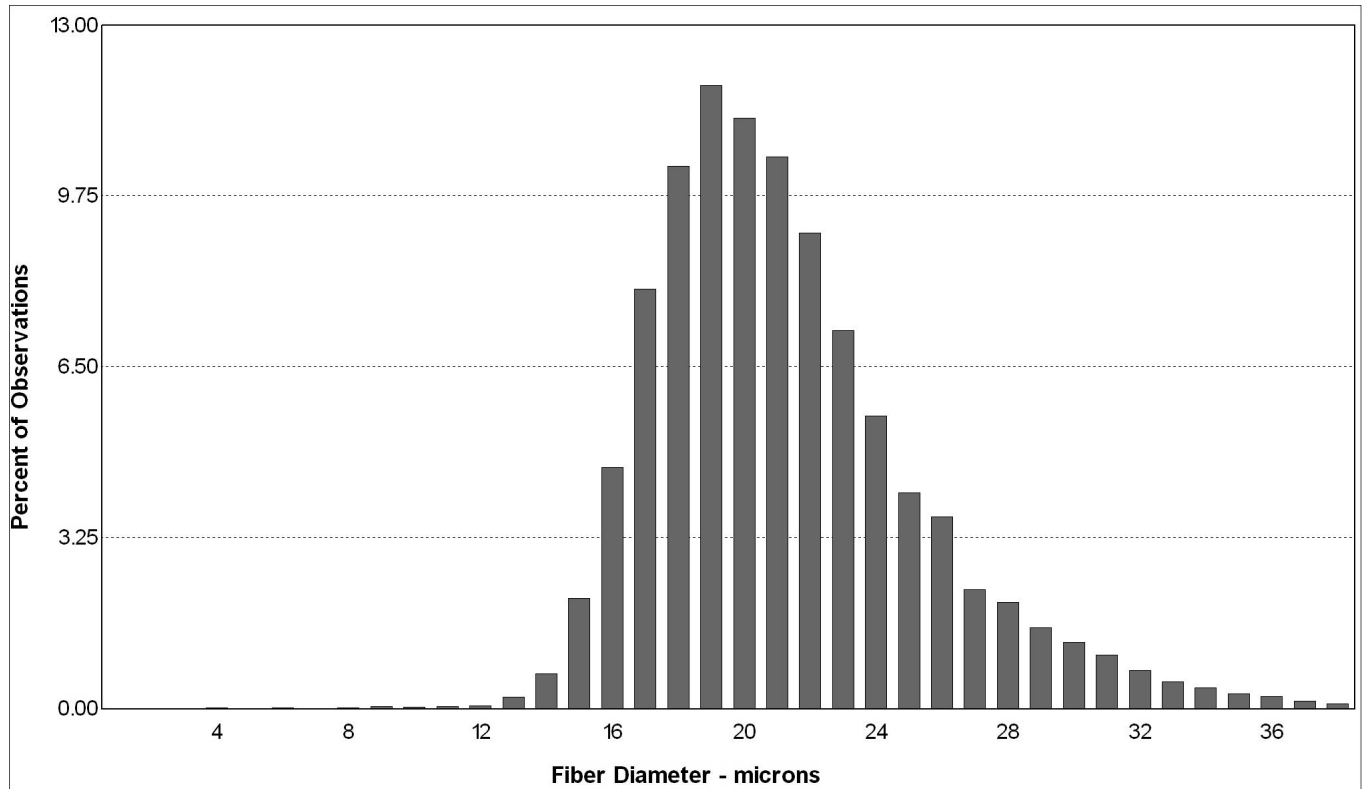

This Test Performed According to I.W.T.O Method 47